

Operating Instructions

Condumax CLS15D/16D/21D

Sensors with Memosens protocol
For conductive measurement of conductivity in liquids

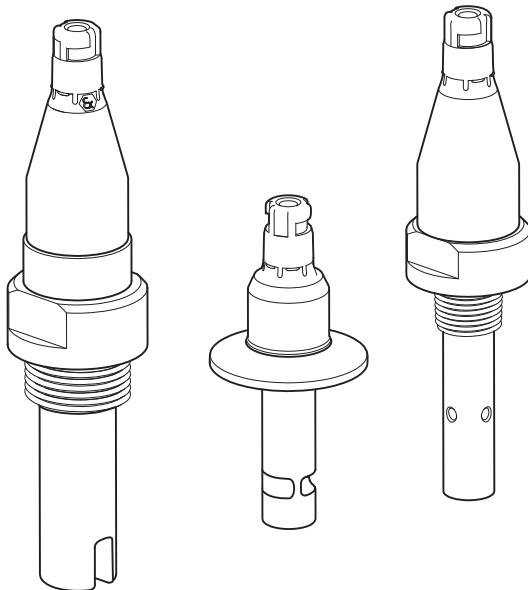


Table of contents

1	Document information	4
1.1	Warnings	4
1.2	Symbols	4
2	Basic safety instructions	5
2.1	Requirements for personnel	5
2.2	Designated use	5
2.3	Occupational safety	5
2.4	Operational safety	6
2.5	Product safety	6
3	Incoming acceptance and product identification	9
3.1	Incoming acceptance	9
3.2	Product identification	9
3.3	Scope of delivery	10
3.4	Certificates and approvals	11
4	Installation	12
4.1	Mounting the sensor	12
4.2	Post-installation check	16
5	Electrical connection	16
5.1	Connection conditions	17
5.2	Connecting the sensor	19
5.3	Ensuring the degree of protection	19
5.4	Post-connection check	19
6	Commissioning	20
7	Maintenance	20
8	Repair	21
8.1	Sealing ring replacement and recalibration (CLS16D only)	21
8.2	Return	22
8.3	Disposal	22
9	Technical data	23
10	EU Declaration of conformity	29
10.1	ATEX / NEPSI II 1G Ex ia IIC T3/T4/T6 Ga, IECEx Ex ia IIC T3/T4/T6 Ga	29
10.2	ATEX/NEPSI II 3G Ex ic IIC T3/T4/T6 Gc	30

1 Document information

1.1 Warnings

Structure of information	Meaning
 Causes (/consequences) If necessary, Consequences of non-compliance (if applicable) ▶ Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid the dangerous situation will result in a fatal or serious injury.
 Causes (/consequences) If necessary, Consequences of non-compliance (if applicable) ▶ Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid the dangerous situation can result in a fatal or serious injury.
 Causes (/consequences) If necessary, Consequences of non-compliance (if applicable) ▶ Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in minor or more serious injuries.
 Cause/situation If necessary, Consequences of non-compliance (if applicable) ▶ Action/note	This symbol alerts you to situations which may result in damage to property.

1.2 Symbols

Symbol	Meaning
	Additional information, tips
	Permitted or recommended
	Not permitted or not recommended
	Reference to device documentation
	Reference to page
	Reference to graphic
	Result of a step

2 Basic safety instructions

2.1 Requirements for personnel

- Installation, commissioning, operation and maintenance of the measuring system may be carried out only by specially trained technical personnel.
- The technical personnel must be authorized by the plant operator to carry out the specified activities.
- The electrical connection may be performed only by an electrical technician.
- The technical personnel must have read and understood these Operating Instructions and must follow the instructions contained therein.
- Faults at the measuring point may only be rectified by authorized and specially trained personnel.



Repairs not described in the Operating Instructions provided must be carried out only directly at the manufacturer's site or by the service organization.

2.2 Designated use

The conductivity sensors are designed for the conductive measurement of the conductivity of liquids.

They are used in the following fields:

Sensor	Applications	Hazardous areas
Condumax CLS15D	Measurements in pure and ultrapure water	Approved for Ex zone 0
Condumax CLS16D	Measurements in pure and ultrapure water with hygienic requirements	Approved for Ex zone 0
Condumax CLS21D	Measurements in media with medium or high conductivity	Approved for Ex zone 0

Use of the device for any purpose other than that described, poses a threat to the safety of people and of the entire measuring system and is therefore not permitted.

The manufacturer is not liable for damage caused by improper or non-designated use.

2.3 Occupational safety

As the user, you are responsible for complying with the following safety conditions:

- Installation guidelines
- Local standards and regulations
- Regulations for explosion protection

Electromagnetic compatibility

- The product has been tested for electromagnetic compatibility in accordance with the applicable European standards for industrial applications.
- The electromagnetic compatibility indicated applies only to a product that has been connected in accordance with these Operating Instructions.

2.4 Operational safety

1. Before commissioning the entire measuring point, verify that all connections are correct. Ensure that electrical cables and hose connections are undamaged.
2. Do not operate damaged products, and safeguard them to ensure that they are not operated inadvertently. Label the damaged product as defective.
3. If faults cannot be rectified:
Take the products out of operation and safeguard them to ensure that they are not operated inadvertently.

2.5 Product safety

2.5.1 State of the art

The product is designed to meet state-of-the-art safety requirements, has been tested, and left the factory in a condition in which it is safe to operate. The relevant regulations and European standards have been observed.

2.5.2 Electrical equipment in hazardous areas

ATEX / NEPSI II 1G Ex ia IIC T3/T4/T6 Ga, IECEx Ex ia IIC T3/T4/T6 Ga

- The Memosens inductive sensor-cable connection system is suitable for use in hazardous areas in accordance with EC type examination certificate BVS 04 ATEX E 121 X. The corresponding EC declaration of conformity is part of this document.
- The certified conductivity sensors CLS15D/CLS16D/CLS21D may only be connected via the measuring cable CYK10-G/I*** to the certified intrinsically safe digital sensor output circuits of measuring device Liquiline M CM42-KE/F/G/I/J***** in accordance with EC type-examination certificate TÜV 13 ATEX 7459 X.
- The electrical connection must be made according to the wiring diagram of the transmitter.
- Metallic process connection parts must be mounted at the mounting location electrostatically conductive ($< 1 \text{ M}\Omega$).
- The CLS15D-type sensors with non-metal process connections and the CLS21D-type sensors may only be employed for measurement in liquids with a minimum conductivity of 10 nS/cm .
- The CLS15D-type sensors with non-metal process connections may not be operated under process conditions in which electrostatic charging of the sensor, and particularly of the electrically insulated outer electrode, is likely to occur.
- Measuring cable CYK10-G/I*** and its terminal head must be protected against electrostatic charging if it is run through Zone 0.
- The maximum permitted cable length is 100 m.
- Ex versions of digital sensors with Memosens technology are indicated by an orange-red ring.
- Full compliance with regulations for electrical systems in hazardous areas (e.g. EN/IEC 60079-14) is mandatory when using the devices and sensors.

Temperature classes

Name	Type					Medium temp. T _a for temperature class (T _n)	Cat.
Condumax	CLS15D	-	A	**	G	-20 °C ≤ T _a ≤ +135 °C (T3) -20 °C ≤ T _a ≤ +120 °C (T4) -20 °C ≤ T _a ≤ +70 °C (T6)	II 1G
Condumax	CLS15D	-	B/L	**	G	-20 °C ≤ T _a ≤ +135 °C (T3) -20 °C ≤ T _a ≤ +100 °C (T4) -20 °C ≤ T _a ≤ +50 °C (T6)	II 1G
Condumax	CLS16D	-	**	**	G	-5 °C ≤ T _a ≤ +135 °C (T3) -5 °C ≤ T _a ≤ +115 °C (T4) -5 °C ≤ T _a ≤ +65 °C (T6)	II 1G
Condumax	CLS21D	-	*	**	G	-20 °C ≤ T _a ≤ +135 °C (T3) -20 °C ≤ T _a ≤ +115 °C (T4) -20 °C ≤ T _a ≤ +65 °C (T6)	II 1G

If the specified medium temperatures are complied with, temperatures that are not permitted for the respective temperature class will not occur on the equipment.

ATEX/NEPSI II 3G Ex ic IIC T3/T4/T6 Gc

- The Memosens inductive sensor-cable connection system is suitable for use in hazardous areas, Zone 2. The corresponding EU declaration of conformity is part of this document.
- The certified conductivity sensors CLS15D / CLS16D / CLS21D may only be connected via the measuring cable CYK10-V*** to the certified intrinsically safe digital sensor output circuits of measuring device Liquiline M CM42-KV*****.
- The electrical connection must be made according to the wiring diagram of the transmitter.
- Metallic process connection parts must be mounted at the mounting location electrostatically conductive (< 1 MΩ).
- The CLS15D-type sensors with non-metal process connections and the CLS21D-type sensors may only be employed for measurement in liquids with a minimum conductivity of 10 nS/cm.
- The CLS15D-type sensors with non-metal process connections may not be operated under process conditions in which electrostatic charging of the sensor, particularly of the electrically insulated outer electrode, is likely to occur.
- The maximum permitted cable length is 100 m.
- Full compliance with regulations for electrical systems in hazardous areas (EN/IEC 60079-14) is mandatory when using the devices and sensors.

Temperature classes

Name	Type					Medium temp. T _a for temperature class (T _n)	Cat.
Condumax	CLS15D	-	A	**	V	-20 °C ≤ T _a ≤ +135 °C (T3) -20 °C ≤ T _a ≤ +120 °C (T4) -20 °C ≤ T _a ≤ +70 °C (T6)	II 3G
Condumax	CLS15D	-	B/L	**	V	-20 °C ≤ T _a ≤ +135 °C (T3) -20 °C ≤ T _a ≤ +100 °C (T4) -20 °C ≤ T _a ≤ +50 °C (T6)	II 3G

Name	Type					Medium temp. T _a for temperature class (Tn)	Cat.
Condumax	CLS16D	-	**	**	V	-5 °C ≤ Ta ≤ +135 °C (T3) -5 °C ≤ Ta ≤ +115 °C (T4) -5 °C ≤ Ta ≤ +65 °C (T6)	II 3G
Condumax	CLS21D	-	*	**	V	-20 °C ≤ Ta ≤ +135 °C (T3) -20 °C ≤ Ta ≤ +115 °C (T4) -20 °C ≤ Ta ≤ +65 °C (T6)	II 3G

If the specified medium temperatures are complied with, temperatures that are not permitted for the respective temperature class will not occur on the equipment.

FM/CSA IS/NI Cl.1 Div.1&2 Gr. A-D

Observe the documentation and the control drawings of the transmitter.

3 Incoming acceptance and product identification

3.1 Incoming acceptance

1. Verify that the packaging is undamaged.
 - ↳ Notify your supplier of any damage to the packaging.
Keep the damaged packaging until the matter has been settled.
2. Verify that the contents are undamaged.
 - ↳ Notify your supplier of any damage to the delivery contents.
Keep the damaged products until the matter has been settled.
3. Check the delivery for completeness.
 - ↳ Check it against the delivery papers and your order.
4. Pack the product for storage and transportation in such a way that it is protected against impact and moisture.
 - ↳ The original packaging offers the best protection.
The permitted ambient conditions must be observed (see "Technical data").

If you have any questions, please contact your supplier or your local sales center.

3.2 Product identification

3.2.1 Type code for versions with explosion protection

Name	Type	Version			
Condumax	CLS15D	-	*	**	G
	CLS16D	-	**	**	G
	CLS21D	-	*	**	G
			Process connections, materials not Ex-relevant		For use in hazardous areas, ATEX/NEPSI II 1G Ex ia IIC T3/T4/T6 Ga, IECEx Ex ia IIC T3/T4/T6 Ga

Name	Type	Version			
Condumax	CLS15D	-	*	**	O
	CLS16D	-	**	**	O
	CLS21D	-	*	**	O
			Process connections, materials not Ex-relevant		For use in hazardous areas, FM/CSA IS/Ni Cl I Div.1&2 Gr. A-D

Name	Type	Version			
Condumax	CLS15D	-	*	**	V
	CLS16D	-	**	**	V
	CLS21D	-	*	**	V
			Process connections, materials not Ex-relevant		For use in hazardous areas, ATEX/NEPSI II 3G Ex ic IIC T3/T4/T6 Gc

3.2.2 Nameplate

The nameplate provides you with the following information on your device:

- Manufacturer identification
 - Extended order code
 - Serial number
 - Safety information and warnings
 - Cell constant (nominal value)
 - Protection class
 - Ex labeling on hazardous area versions
- Compare the data on the nameplate with your order.

3.2.3 Product identification

Product page

www.endress.com/cls15d

www.endress.com/cls16d

www.endress.com/cls21d

Interpreting the order code

The order code and serial number of your product can be found in the following locations:

- On the nameplate
- In the delivery papers

Obtaining information on the product

1. Go to the product page for your product on the Internet.
2. At the bottom of the page, select the "Online Tools" link followed by "Check your device features".
 - ↳ An additional window opens.
3. Enter the order code from the nameplate into the search field, and then select "Show details".
 - ↳ You will receive information on each feature (selected option) of the order code.

Manufacturer's address

Endress+Hauser Conducta GmbH+Co. KG
Dieselstraße 24
D-70839 Gerlingen

3.3 Scope of delivery

The scope of delivery includes:

- Sensor in the version ordered
- Operating Instructions

3.4 Certificates and approvals

3.4.1 CE mark

Declaration of conformity

The product meets the requirements of the harmonized European standards. As such, it complies with the legal specifications of the EU directives. The manufacturer confirms successful testing of the product by affixing to it the **CE** mark.

3.4.2 Hazardous area approvals

ATEX / NEPSI II 1G Ex ia IIC T3/T4/T6 Ga, IECEx Ex ia IIC T3/T4/T6 Ga
FM/CSA IS/Ni Cl. I Div.1&2 Gr. A-D in conjunction with Liquiline M CM42 transmitter
ATEX/NEPSI II 3G Ex ic IIC T3/T4/T6 Gc for use in Zone 2 with Liquiline M CM42-KV***
transmitter



ATEX and FM/CSA versions of digital sensors with Memosens technology are indicated by a red-orange ring in the plug-in head.

3.4.3 EHEDG (CLS16D only)

Validated as follows:

- Cleanability in accordance with EHEDG, Document 2
- Sterilizability in accordance with EHEDG, Document 5
- Bacteria-tightness in accordance with EHEDG, Document 7

3.4.4 FDA (CLS16D only)

All materials in contact with the product are listed by the FDA.

3.4.5 Manufacturer inspection certificate

Stating the individual cell constant

3.4.6 Biological reactivity test (USP class VI, CLS16D only)

Biological reactivity test certificate according to USP (United States Pharmacopeia) part <87> and part <88> class VI with batch traceability of materials in contact with the medium

3.4.7 Inspection certificate in accordance with EN 10204 3.1

A test certificate 3.1 in accordance with EN10204 is supplied depending on the version (→ Product Configurator on the product page).

3.4.8 ASME (CLS16D only)

Manufactured in accordance with ASME criteria (American Society of Mechanical Engineers)

3.4.9 Certification body


DEKRA EXAM GmbH
Bochum

4 Installation

4.1 Mounting the sensor

4.1.1 CLS15D

The sensors are installed directly via the process connection thread NPT 1/2" or 3/4" or clamp 1 1/2". As an option, the sensor can also be installed using a commercially available T-piece or cross fitting or using a flow assembly.

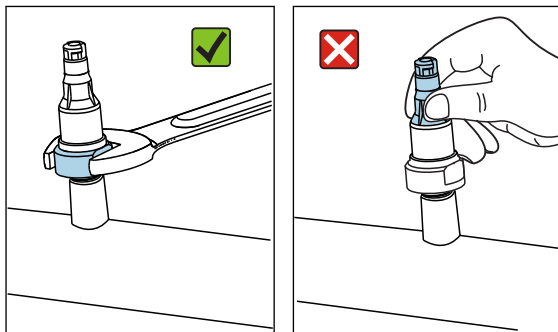


NOTICE

Incorrect mounting or disassembly

The Memosens head could become loose and fall off, resulting in total sensor failure


- Only mount the sensor via the process connection.
- To do so, use a suitable tool, such as an open-ended wrench.

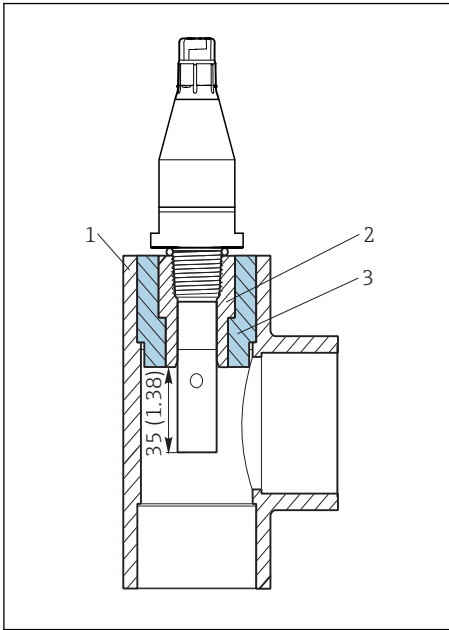

A0019015

- 1 With NPT 1/2" thread in T-piece or cross fitting

- 1 T-piece or cross fitting (DN 32, 40 or 50)
- 2 Glue-in VC threaded coupling (NPT 1/2" for DN 20)
- 3 Glue-in adapter coupling (for DN 32, 40, 50)

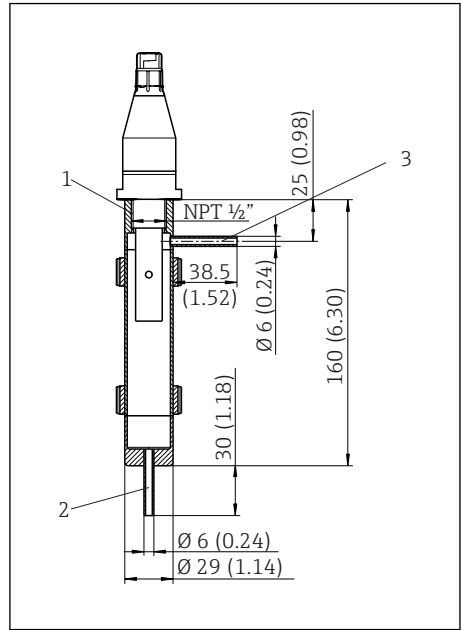

A0019014


- 2 With NPT 1/2" thread in flow assembly 71042405, dimensions in mm (inch)

- 1 Sensor holder NPT 1/2"
- 2 Inlet
- 3 Outlet


i Ensure that the electrodes are fully immersed in the medium during measurement. The immersion depth must be at least 35 mm (1.38"). If the sensor is being used in the ultrapure water range, you must work under air-evacuated conditions. Otherwise the CO₂ in the air can dissolve in the water and its (weak) dissociation can increase the conductivity by up to 3 µS/cm.

4.1.2 CLS16D

The sensors are installed directly via the process connection. Take the flow direction into consideration when installing in pipes.

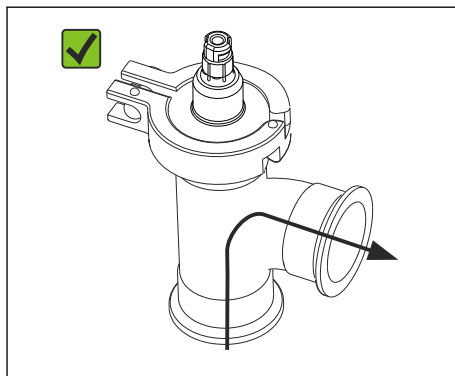

3 Permitted flow direction

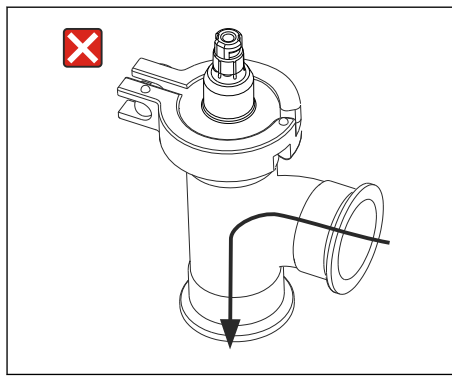

4 Inadmissible flow direction



Ensure that the electrodes are fully immersed in the medium during measurement. If the sensor is being used in the ultrapure water range, you must work under air-evacuated conditions. Otherwise the CO_2 in the air can dissolve in the water and its (weak) dissociation can increase the conductivity by up to $3 \mu\text{S}/\text{cm}$.


4.1.3 CLS21D



Clamp connection

Both sheet-metal brackets and solid brackets can be used to secure the sensor. Sheet-metal brackets have a lower dimensional stability, uneven bearing surfaces causing point loads, and sometimes sharp edges that can damage the clamp. We recommend you only use solid brackets due to their higher dimensional stability. Solid brackets can be used over the entire pressure/temperature range (see pressure-temperature ratings).

The sensors are installed directly via the process connection. As an option, the sensor can also be installed via a flow assembly.

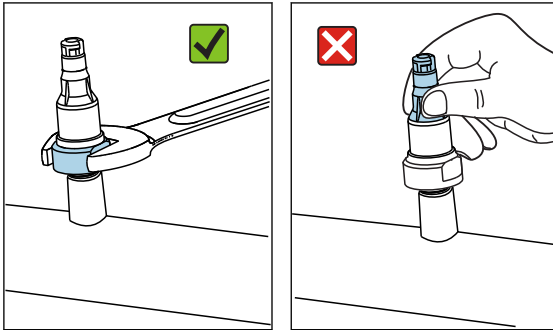


NOTICE

Incorrect mounting or disassembly


The Memosens head could become loose and fall off, resulting in total sensor failure

- Only mount the sensor via the process connection.
- To do so, use a suitable tool, such as an open-ended wrench.

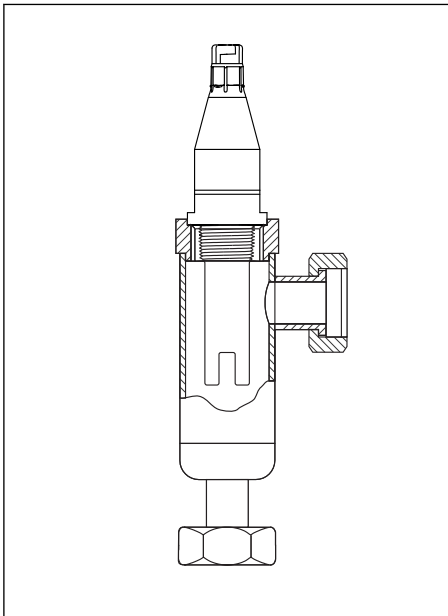

A0019019


5 Installation in flow assembly CLA751

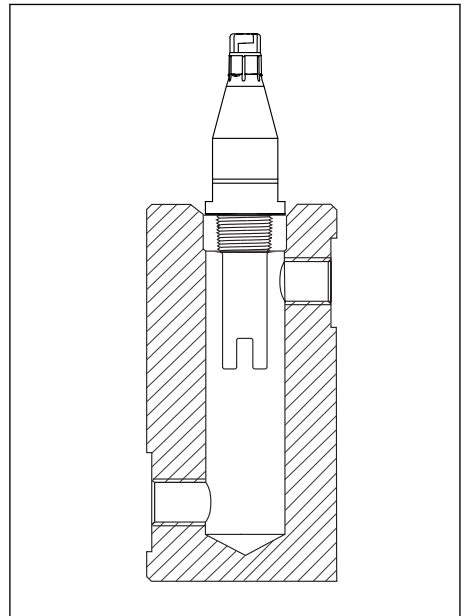

A0019020

6 Installation in flow assembly CLA752

The Dipfit CLA111 immersion assembly is available to install sensors with a G1 thread in vessels.

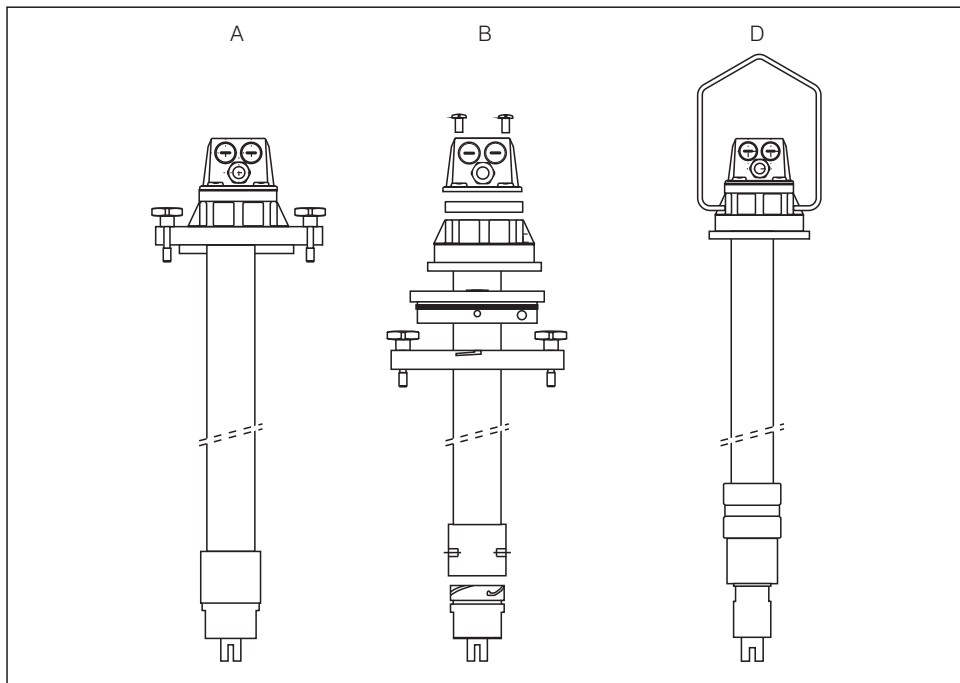

A0024145

 7 Installation in Dipfit CLA111 immersion assembly, fastening versions A, B and D

 Ensure that the electrodes are fully immersed in the medium during measurement.

4.2 Post-installation check

- Are the sensor and cable undamaged?
- Is the sensor installed in the process connection and is not suspended from the cable?

5 Electrical connection

WARNING

Device is live


Incorrect connection may result in injury or death

- ▶ The electrical connection may be performed only by an electrical technician.
- ▶ The electrical technician must have read and understood these Operating Instructions and must follow the instructions contained therein.
- ▶ **Prior** to commencing connection work, ensure that no voltage is present on any cable.

5.1 Connection conditions

5.1.1 Connection at a glance


Sensors for zone 0

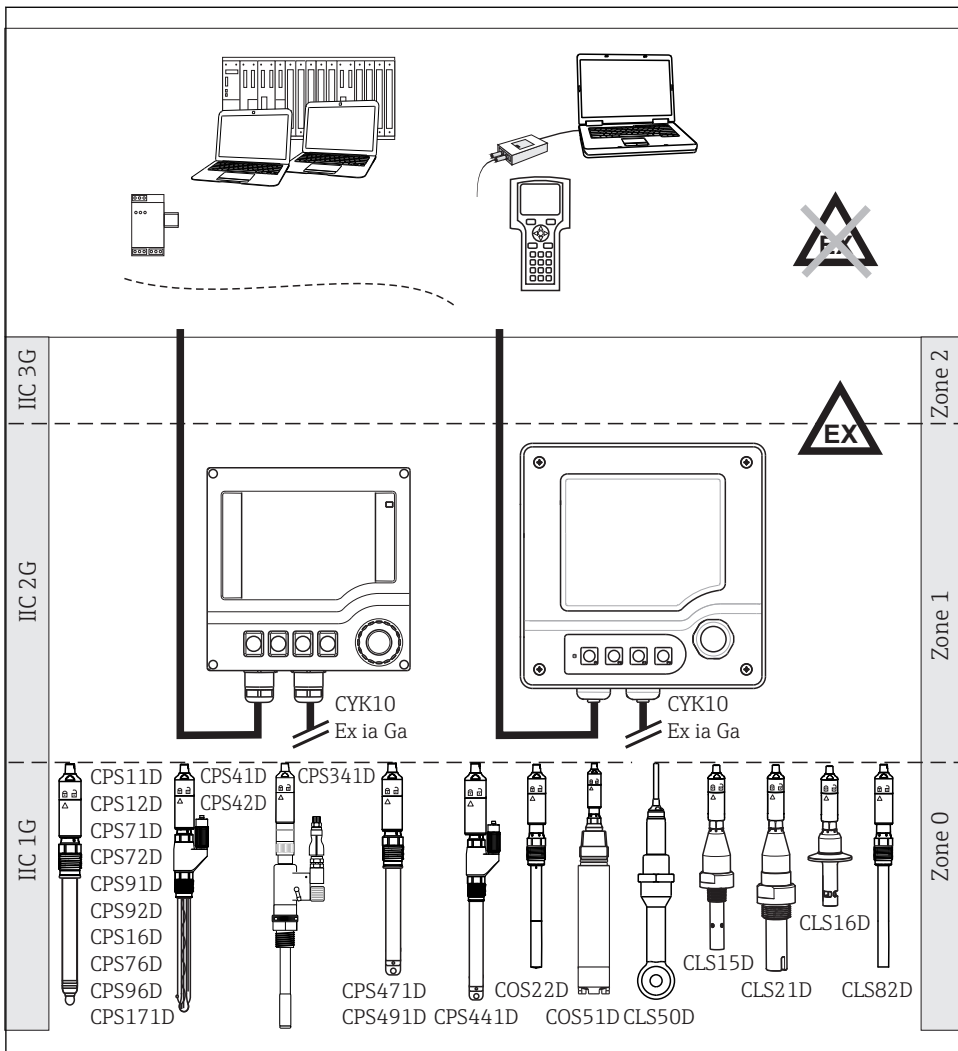

8 Electrical connection in hazardous environment

A0031174

Sensors for zone 2

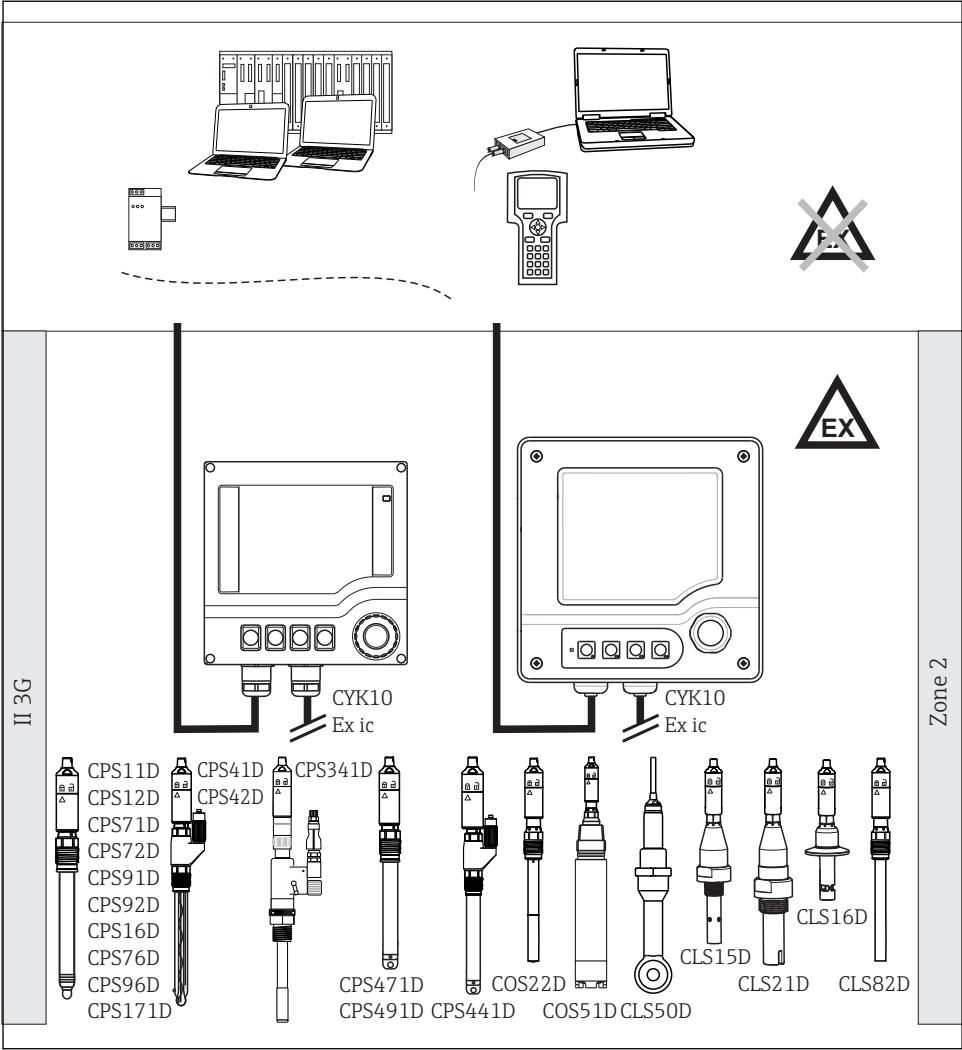


9 Electrical connection in hazardous environment

A0031184

5.2 Connecting the sensor

The electrical connection of the sensor to the transmitter is performed using the measuring cable CYK10.

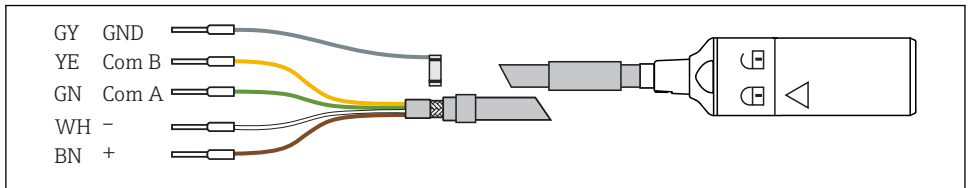

A0024019

 10 Measuring cable CYK10

NOTICE

Mechanical twist protection for CLS15D and CLS21D

If too much force is applied to the Memosens head, this can shear the connections and therefore destroy the sensor

- ▶ There is no need to exert excessive force when connecting the sensor to the cable coupling. Always connect the sensor gently.
- ▶ If the Memosens coupling clearly will not close, check the coupling for dirt or mechanical damage and make sure you are turning in the right direction. Pay attention to the lock symbol on the coupling.
- ▶ Use another Memosens cable if necessary.

5.3 Ensuring the degree of protection

Only the mechanical and electrical connections which are described in these instructions and which are necessary for the required, designated use, may be carried out on the device delivered.

- ▶ Exercise care when carrying out the work.

Otherwise, the individual types of protection (Ingress Protection (IP), electrical safety, EMC interference immunity) agreed for this product can no longer be guaranteed due, for example, to covers being left off or cable (ends) which are loose or insufficiently secured.

5.4 Post-connection check

Device condition and specifications	Notes
Are the outside of the sensor, assembly, cable undamaged?	Visual inspection
Electrical connection	Notes
Are the installed cables strain-relieved and not twisted?	
Is a sufficient length of the cable cores stripped, and is it positioned in the terminal correctly?	Check the fit (by pulling gently)
Are all the screws terminals properly tightened?	Tighten

Device condition and specifications	Notes
Are all cable entries mounted, tightened and leak-tight?	For lateral cable entries, make sure the cables loop downwards to allow water to drip off
Are all cable entries installed downwards or mounted laterally?	

6 Commissioning

Before first commissioning, check if:

- the sensor is correctly installed
- the electrical connection is correct.

If using an assembly with automatic cleaning, check that the cleaning medium (e.g. water or air) is connected correctly.

WARNING

Escaping process medium

Risk of injury from high pressure, high temperatures or chemical hazards

- ▶ Before applying compressed air to an assembly with cleaning facility, make sure the connections are correctly fitted.
- ▶ Do not install the assembly in the process if you cannot make the correct connection reliably.

7 Maintenance

CAUTION

Corrosive chemicals

Danger of chemical burns to the eyes and skin. Danger of damage to clothing and equipment

- ▶ It is absolutely essential to protect the eyes and hands properly when working with acids, bases and organic solvents!
- ▶ Wear protective goggles and safety gloves.
- ▶ Clean away splashes on clothes and other objects to prevent any damage.
- ▶ Pay particular attention to the information provided in the safety data sheets for the chemicals used.

WARNING

Hydrofluoric acid and mineral acids

Risk of serious or fatal injury from caustic burns

- ▶ Wear protective goggles to protect your eyes.
- ▶ Wear protective gloves and appropriate protective clothing.
- ▶ Avoid all contact with the eyes, mouth and skin.
- ▶ If using hydrofluoric acid, only use plastic vessels.

⚠ WARNING**Thiocarbamide**

Harmful if swallowed. Limited evidence of carcinogenicity. Possible risk of harm to the unborn child. Dangerous for the environment with long-term effects.

- ▶ Wear protective goggles, protective gloves and appropriate protective clothing.
- ▶ Avoid all contact with the eyes, mouth and skin.
- ▶ Avoid releases into the environment.

Clean away fouling on the sensor as follows depending on the type of fouling:

1. Oily and greasy films:
Clean with grease remover, e.g. alcohol, as well as hot water and (alkaline) agents containing surfactants (e.g. dishwashing detergent).
2. Lime, cyanide and metal hydroxide buildup and low solubility organic buildup:
Dissolve buildup with diluted hydrochloric acid (3 %) and then rinse thoroughly with plenty of clear water.
3. Sulfidic buildup (from flue gas desulfurization or sewage treatment plants):
Use a mixture of hydrochloric acid (3 %) and thiocarbamide (commercially available) and then rinse thoroughly with plenty of clear water.
4. Buildup containing proteins (e.g. food industry):
Use a mixture of hydrochloric acid (0.5 %) and pepsin (commercially available) and then rinse thoroughly with plenty of clear water.
5. Readily soluble biological buildup:
Rinse with pressurized water.



After cleaning or regeneration, you must rinse the sensor thoroughly with water and then recalibrate it.

8 Repair

8.1 Sealing ring replacement and recalibration (CLS16D only)

Intact seals are a prerequisite for safe and reliable measurements. The seal should be replaced at regular intervals to guarantee maximum sensor operational safety and hygiene.

Practical repair intervals can only be determined by the user as they depend greatly on the operating conditions, such as:

- Type and temperature of the product
- Type and temperature of the cleaning agent
- Number of cleanings
- Number of sterilizations
- Operating environment

Recommended intervals for seal replacement (reference values)

Application	Window
Media with temperatures from 50 to 100 °C (122 to 212 °F)	Approx. 18 months
Media with temperatures < 50 °C (122 °F)	Approx. 36 months
Sterilization cycles, max. 150 °C (302 °F), 45 min.	Approx. 400 cycles

To ensure your sensor is operational again after being exposed to very high loads, you can have it regenerated in the factory. In the factory, the sensor is fitted with new seals and recalibrated.

Please contact your sales office for information on replacing the seal and recalibration in the factory.

8.2 Return

The product must be returned if repairs or a factory calibration are required, or if the wrong product was ordered or delivered. As an ISO-certified company and also due to legal regulations, Endress+Hauser is obliged to follow certain procedures when handling any returned products that have been in contact with medium.

To ensure swift, safe and professional device returns, please read the return procedures and conditions at www.endress.com/support/return-material.

8.3 Disposal

The device contains electronic components and must therefore be disposed of in accordance with regulations on the disposal of electronic waste.

Observe the local regulations.

9 Technical data

9.1 Input

9.1.1 Measured values

- Conductivity
- Temperature

9.1.2 Measuring ranges

Conductivity	(in relation to water at 25 °C (77 °F))
CLS15D-A	0.04 to 20 µS/cm
CLS15D-B/L	0.10 to 200 µS/cm
CLS16D	0.04 to 500 µS/cm
CLS21D	10 µS/cm to 20 mS/cm
Temperature	
CLS15D	-20 to 100 °C (-4 to 212 °F)
CLS16D	-5 to 100 °C (23 to 212 °F)
CLS21D	-20 to 100 °C (-4 to 212 °F)

9.1.3 Cell constant

CLS15D-A	$k = 0.01 \text{ cm}^{-1}$
CLS15D-B/L	$k = 0.1 \text{ cm}^{-1}$
CLS16D	$k = 0.1 \text{ cm}^{-1}$
CLS21D	$k = 1.0 \text{ cm}^{-1}$, nominal

9.1.4 Temperature compensation

NTC 30K

9.2 Performance characteristics

9.2.1 Uncertainty of measurement

CLS15D

Each individual sensor is factory-measured in a solution of approx. 5 µS/cm for cell constant 0.01 cm⁻¹ or approx. 50 µS/cm for cell constant 0.1 cm⁻¹ using a reference measuring system traceable to NIST or PTB. The exact cell constant is entered into the quality certificate supplied. The uncertainty of measurement in determining the cell constant is 1.0 %.

CLS16D

Each individual sensor is factory-measured in a solution of approx. 5 µS/cm using a reference measuring system traceable to NIST or PTB. The exact cell constant is entered into the quality certificate supplied. The uncertainty of measurement in determining the cell constant is 1.0 %.

CLS21D

Each individual sensor is factory-measured in a solution of approx. 5 mS/cm using a reference measuring system traceable to NIST or PTB. The exact cell constant is entered into the quality certificate supplied. The uncertainty of measurement in determining the cell constant is 1.0 %.

9.2.2 Response time

Conductivity	$t_{95} \leq 3 \text{ s}$
Temperature	
CLS15D-A	$t_{90} \leq 39 \text{ s}$
CLS15D-B/L	$t_{90} \leq 17 \text{ s}$
CLS16D	$t_{90} \leq 13 \text{ s}$
CLS21D	$t_{90} \leq 296 \text{ s}$

9.2.3 Maximum measured error

CLS15D	2% of reading
CLS16D	2 % of reading up to 200 µS/cm 3 % of reading from 200 to 500 µS/cm
CLS21D	5% of reading

9.2.4 Repeatability

0.2% of reading

9.3 Environment

9.3.1 Ambient temperature range

-20 to +60 °C (-4 to 140 °F)

9.3.2 Storage temperature

-25 to +80 °C (-10 to +180 °F)

9.3.3 Degree of protection

IP 68 / NEMA type 6P (1 m water column, 25 °C, 24 h)

9.4 Process

9.4.1 Process temperature

CLS15D

Normal operation

-20 to 120 °C (-4 to 248 °F)

Sterilization (max. 1 h) ¹⁾

Max. 140 °C (284 °F)

CLS16D

Normal operation

-5 to 120 °C (23 to 248 °F)

Sterilization (max. 45 min)

Max. 150 °C (302 °F) at 6 bar (87 psi) absolute

CLS21D

-20 to +135 °C (-4 to 275 °F) at 3.5 bar (50 psi) absolute

1) Threaded versions: max. 30 minutes



The maximum temperature for communication with the transmitter is 130 °C (266°F) for the Memosens versions.

9.4.2 Process pressure

CLS15D

13 bar (188 psi) absolute, at 20 °C (68 °F)

2 bar (29 psi) absolute, at 120 °C (248 °F)

CLS16D

13 bar (188 psi) absolute, at 20 °C (68 °F)

9 bar (130 psi) absolute, at 120 °C (248 °F)


0.1 bar (1.5 psi) absolute (negative pressure), at 20 °C (68 °F)

CLS21D

17 bar (246 psi) absolute, at 20 °C (68 °F)

9.4.3 Temperature/pressure ratings

CLS15D

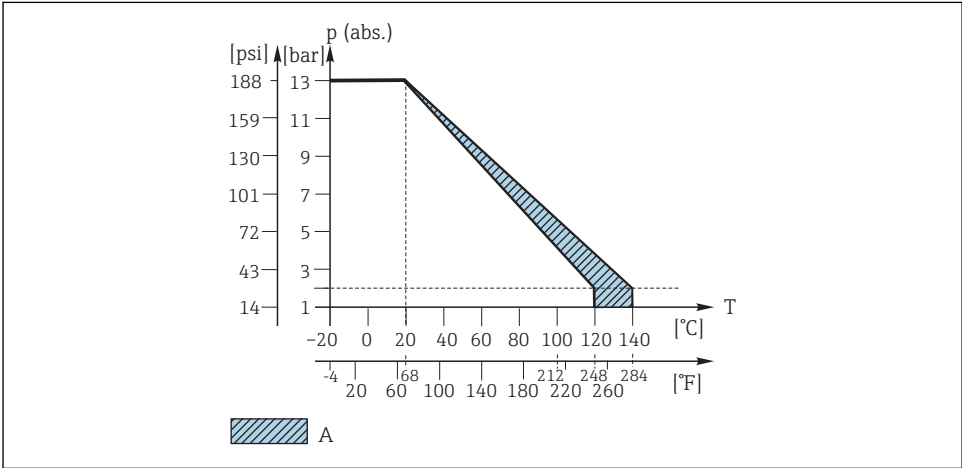


A0031428-EN

11 Mechanical pressure-temperature resistance

A Can be sterilized for a short time (1 hour)

CLS16D

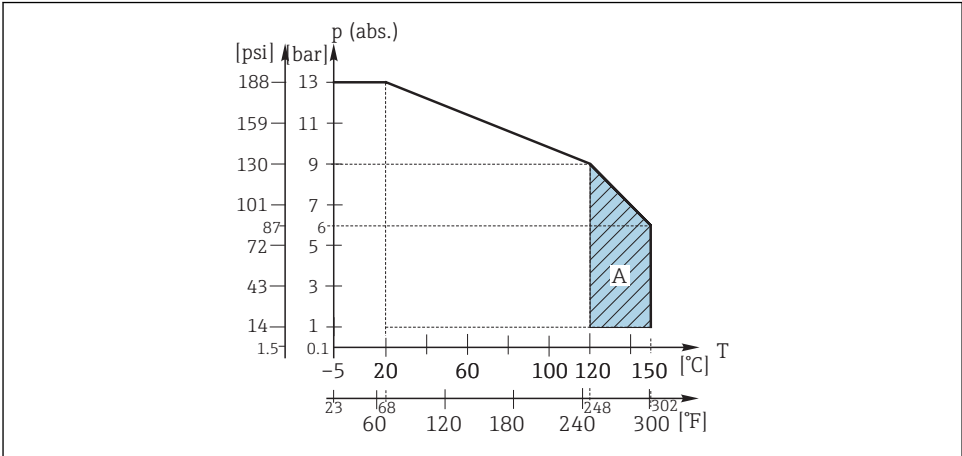


A0031431-EN

12 Mechanical pressure-temperature resistance

A Can be sterilized for a short time (45 min.)

CLS21D

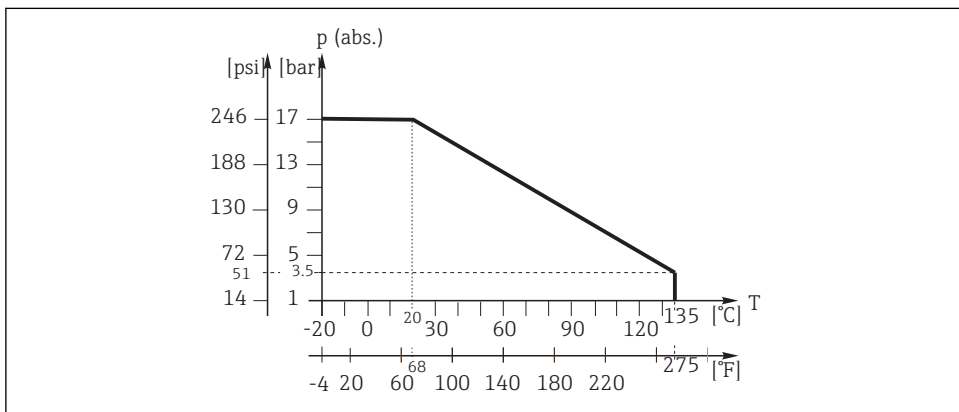

A0031435-EN

13 Mechanical pressure-temperature resistance

9.5 Mechanical construction

9.5.1 Weight

CLS15D and CLS21D

Approx. 0.3 kg (0.66 lbs) depending on version

CLS16D

Approx. 0.13 to 0.75 kg (0.29 to 1.65 lbs) depending on version

9.5.2 Materials

CLS15D

Electrodes	Polished, stainless steel 1.4435 (AISI 316L)
Sensor shaft	Polyethersulfone (PES-GF20)
O-ring, in contact with medium (only Clamp version)	EPDM

CLS16D

Electrodes	Electropolished, stainless steel 1.4435 (AISI 316L)
Seal	Gasket seal ISOLAST (FFKM), FDA-compliant

CLS21D

Electrodes	Graphite
Sensor shaft	Polyethersulfone (PES-GF20)
Thermal conductivity socket for temperature probe	Titanium 3.7035

9.5.3 Process connection

CLS15D

Thread NPT ½" and ¾"

Clamp 1½" as per ISO 2852

CLS16D

Clamp 1", 1½", 2" as per ISO 2852 (also suitable for TRI-CLAMP, DIN 32676)

Tuchenhagen VARIVENT N DN 50 to 125

NEUMO BioControl D50

CLS21D

Thread G1

NPT 1" thread

Clamp 2" as per ISO 2852

Sanitary connection DN 25 as per DIN 11851

9.5.4 Surface roughness (CLS15D, CLS16D only)

CLS15D

$R_a \leq 0.8 \mu\text{m}$


CLS16D

$R_a \leq 0.8 \mu\text{m}$, electropolished


$R_a \leq 0.38 \mu\text{m}$, electropolished, optional

10 EU Declaration of conformity

10.1 ATEX / NEPSI II 1G Ex ia IIC T3/T4/T6 Ga, IECEx Ex ia IIC T3/T4/T6 Ga

EG/EU-Konformitätserklärung EC/EU-Declaration of Conformity Déclaration CE/UE de Conformité		Endress+Hauser  People for Process Automation	
			
Company	Endress+Hauser Conducta GmbH+Co. KG Dieselstraße 24, 70839 Gerlingen, Germany erklärt als Hersteller in alleiniger Verantwortung, dass das Produkt declares as manufacturer under sole responsibility, that the product déclare sous sa seule responsabilité en qualité de fabricant que le produit		
Product	Memosens CLS15D-***G CLS16D-****G CLS21D-***G zusammen mit Messkabel / together with measuring cable / ensemble avec cable de mesure CYK10-a**b a = G, E; b = 1, 2 CYK20-BAab a = B1, B2; b = C1, C2		
Regulations	den folgenden Europäischen Richtlinien entspricht: conforms to following European Directives: est conforme aux prescriptions des Directives Européennes suivantes : EMC 2014/30/EU ATEX 2014/34/EU		
Standards	angewandte harmonisierte Normen oder normative Dokumente: applied harmonized standards or normative documents: normes harmonisées ou documents normatifs appliqués : EN 61326-1 (2013) EN 60079-0 (2012) + A11 (2013) EN 61326-2-3 (2013) EN 60079-11 (2012) EN 60079-26 (2007) + Corrigendum 1		
Certification	EG-Baumusterprüfbescheinigungs-Nr. BVS 04 ATEX E 121 X EC-Type Examination Certificate No. Numéro de l'attestation d'examen CE de type Ausgestellt von/issued by/délivré par DEKRA EXAM GmbH (0158) Qualitätssicherung/Quality assurance/Système d'assurance DEKRA EXAM GmbH (0158) qualite Gerlingen, 20.04.2016 Endress+Hauser Conducta GmbH+Co. KG		
	 I. V. Jörg Martin Müller Technology		 I. V. Sven-Matthias Scheibe Technology Certifications and Approvals
EC_00358_01.16			

10.2 ATEX/NEPSI II 3G Ex ic IIC T3/T4/T6 Gc

EG/EU-Konformitätserklärung EC/EU-Declaration of Conformity Déclaration CE/UE de Conformité		Endress+Hauser  People for Process Automation
		
Company	Endress+Hauser Conducta GmbH+Co. KG Dieselstraße 24, 70839 Gerlingen, Germany erklärt als Hersteller in alleiniger Verantwortung, dass das Produkt declares as manufacturer under sole responsibility, that the product déclare sous sa seule responsabilité en qualité de fabricant que le produit	
Product	Memosens Sensoren / Memosens sensors / Memosens capteurs CLS15D-***V CLS16D-***V CLS21D-***V zusammen mit Messkabel / together with measuring cable / ensemble avec cable de mesure CYK10-V**a a = 1, 2 CYK20-BAab a = B1, B2; b = C1, C2	
Regulations	den folgenden Europäischen Richtlinien entspricht: conforms to following European Directives: est conforme aux prescriptions des Directives Européennes suivantes : EMC 2014/30/EU (L96/79) ATEX 2014/34/EU (L96/309)	
Standards	angewandte harmonisierte Normen oder normative Dokumente: applied harmonized standards or normative documents: normes harmonisées ou documents normatifs appliqués : EN 61326-1 (2013) EN 60079-0 (2012) + A11 (2013) EN 61326-2-3 (2013) EN 60079-11 (2012)	
Certification	EG-Baumusterprüfbescheinigungs-Nr. - EC-Type Examination Certificate No. Numéro de l'attestation d'examen CE de type Ausgestellt von/issued by/délivré par - Qualitätssicherung/Quality assurance/Système d'assurance DEKRA EXAM GmbH (0158) qualité Gerlingen, 20.04.2016 Endress+Hauser Conducta GmbH+Co. KG	
	 i. V. Jörg-Martin Müller Technology  i. V. Sven-Matthias Scheibe Technology Certifications and Approvals	
EC_00360_01-16		



71382087

www.addresses.endress.com
